Cordis **EXOSEAL**TM


Vascular Closure Device




Insert

Using fluoroscopy, verify the femoral artery's suitability for arteriotomy closure with the EXOSEAL™ VCD, including the insertion angle (30-45 degrees) of the vascular sheath introducer.

- 1. Insert the EXOSEAL[™] Device into the sheath, advance to the black marker band.
- 2. Retract the sheath back to the wirecowling.
- 3. Continue to retract the sheath compressing the green Indicator Wire Cowling against the white handle. A "click" will be heard.

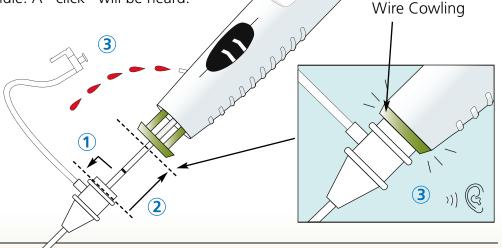


Green Indicator

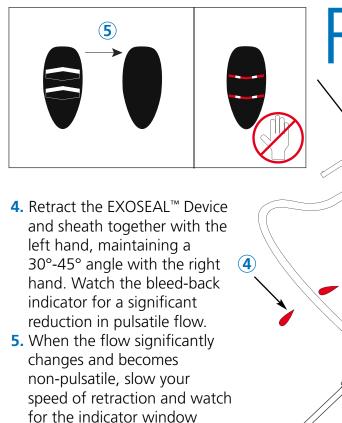


to change to all BLACK.

Retract

- **6.** Press the green plug deployment button fully into the white handle. 7. Remove the EXOSEAL™ Device and sheath together.
- 8. Apply light non-occlusive finger tip pressure at the puncture site for 2 mins. Apply a sterile dressing and then observe site as per hospital protocol.









For Healthcare Professionals Only. Important information: Prior to use, refer to the instructions for use supplied with this device for indications, contraindications, side effects, suggested procedure, warnings and precautions. As part of its continuous product development policy, Cordis reserves the right to change product specifications without prior notification. Please contact your Cordis representative for additional product availability information. CORDIS, Cordis LOGO, EXOSEAL are trademarks of Cardinal Health and may be registered in the US and/or in other countries. © 2020 Cardinal Health. All Rights Reserved. 100572036 11/2020



Please refer to the complete "Instructions For Use" including all the steps to be followed during the procedure (Section XI. Procedure) and the table of compatible sheaths before using the EXOSEALTM Vascular Closure Device (Section X. Sheath Introducers Compatible with EXOSEALTM Vascular Closure Device (VCD)