



# THE ART OF FLOW RESTORATION

**RAIDEN3™**

NON-COMPLIANT PTCA BALLOON



**OVERVIEW**

**HIGH PRESSURE**

**CROSSABILITY**

**CODES**




**RAIDEN3™**  
Non-Compliant PTCA Balloon

**For Both Everyday  
and Complex Cases\***

- Manufactured by Kaneka Corporation, one of Japan's leading providers of interventional devices.
- Part of the PTCA balloon portfolio of Cordis Company.
- **Durable Balloon with Japanese Technology**
- Engineered for small and narrow lesions.

\*Challenging lesions such as calcified or tortuous lesions may not be crossed with this catheter. The physician in charge of the procedure should determine whether this catheter is applicable based on his/her past experiences.







Highest RBP up to 22 atm


Advancing Crossability Performance

High Pressure, Noncompliant Balloon for Confidence in Preserving Post-Dilatation Accuracy


- Japanese Balloon Design.
- Powerful 22 atm RBP.
- Low compliance facilitates post-dilatation accuracy.
- Engineered for strength and puncture resistance.
- Higher pressure facilitates stent tacking.



**HYDROPHILIC COATING**  
Improves lubricity, thereby reducing resistance.



**TAPERED BALLOON SHAPE**  
Features a smooth tip, and a low profile engineered to help to prevent buckling and facilitate crossing.




**TRI-FOLD WRAPPING TECHNOLOGY**  
Optimized balloon-wrapping technology.



**LOW PROFILE 1.5MM DIAMETER POST-DILATATION BALLOON**


BALLOON STRENGTH



Lowest pressure in the graph refers to NP and highest one to RBP.  
RBP: 22atm (ø2.25-4.0mm; 20atm for Ø1.5-2.0mm + 4.25-4.5mm).

\*\* Information related to competitive products was obtained from public sources, including company websites, sales material and related documentation in Sept 2021.


Crossability of 3.0mm Post-Dilatation Products\*

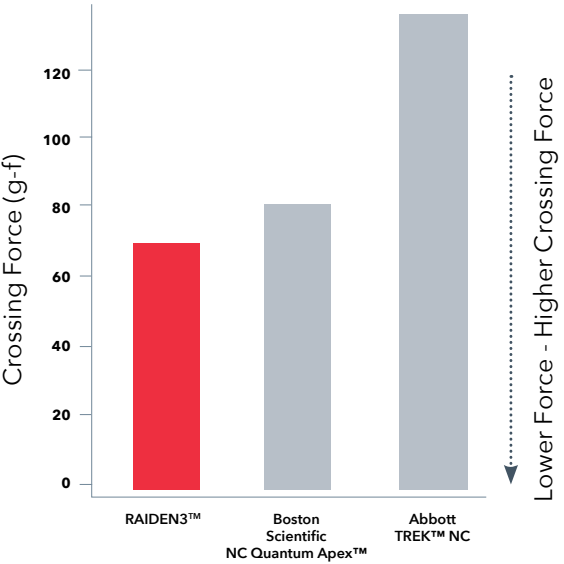

Cordis data on file, 2016



Product Overview and Ordering




Key Specifications	
Effective Length:	146cm
Radiopaque Markers:	1 (ø1.5 - 1.75mm) 2 (ø2.0 - 4.5mm)
Compatible Max Guidewire OD:	0.014"
Balloon Folds:	2-fold (ø1.5 ~ 1.75mm) 3-fold (ø2 ~ 4.5mm)
Accessories:	Flushing tool and Catheter clip

Balloon Diameter (mm)	Balloon Length (mm)	Compatibility Sheath	Nominal Pressure (atm)	Rated Burst Pressure (atm)	Catalog Reference Number
1.50	8	5	12	20	RD3-8-150
1.75	8	5	12	20	RD3-8-175
2.00	8	5	12	20	RD3-8-200
2.00	10	5	12	20	RD3-10-200
2.00	13	5	12	20	RD3-13-200
2.00	15	5	12	20	RD3-15-200
2.00	20	5	12	20	RD3-20-200
2.25	10	5	12	22	RD3-10-225
2.25	13	5	12	22	RD3-13-225
2.25	15	5	12	22	RD3-15-225
2.25	20	5	12	22	RD3-20-225
2.50	8	5	12	22	RD3-8-250
2.50	10	5	12	22	RD3-10-250
2.50	13	5	12	22	RD3-13-250
2.50	15	5	12	22	RD3-15-250
2.50	20	5	12	22	RD3-20-250
2.50	30	5	12	22	RD3-30-250
2.75	10	5	12	22	RD3-10-275
2.75	13	5	12	22	RD3-13-275
2.75	15	5	12	22	RD3-15-275
2.75	20	5	12	22	RD3-20-275
3.00	8	5	12	22	RD3-8-300
3.00	10	5	12	22	RD3-10-300
3.00	13	5	12	22	RD3-13-300
3.00	15	5	12	22	RD3-15-300
3.00	20	5	12	22	RD3-20-300
3.00	30	5	12	22	RD3-30-300
3.25	10	5	12	22	RD3-10-325
3.25	13	5	12	22	RD3-13-325
3.25	15	5	12	22	RD3-15-325
3.25	20	5	12	22	RD3-20-325
3.50	8	5	12	22	RD3-8-350
3.50	10	5	12	22	RD3-10-350
3.50	13	5	12	22	RD3-13-350
3.50	15	5	12	22	RD3-15-350
3.50	20	5	12	22	RD3-20-350
3.50	30	5	12	22	RD3-30-350
3.75	10	5	12	22	RD3-10-375
3.75	13	5	12	22	RD3-13-375
3.75	15	5	12	22	RD3-15-375
3.75	20	5	12	22	RD3-20-375
4.00	8	5	12	22	RD3-8-400
4.00	10	5	12	22	RD3-10-400
4.00	13	5	12	22	RD3-13-400
4.00	15	5	12	22	RD3-15-400
4.00	20	5	12	22	RD3-20-400
4.00	30	5	12	22	RD3-30-400
4.25	10	5	12	20	RD3-10-425
4.25	15	5	12	20	RD3-15-425
4.50	10	5	12	20	RD3-10-450
4.50	13	5	12	20	RD3-13-450
4.50	15	5	12	20	RD3-15-450
4.50	20	5	12	20	RD3-20-450







## RAIDEN3™

### Non-Compliant PTCA Balloon

**WARNINGS:** STERILE product, to be for one-time use only. For single use only. Do not reuse, reprocess or resterilize. Do not inflate the balloon exceeding the diameter of the blood vessel in the vicinity of the stenotic lesion. (The blood vessel may be damaged or ruptured.) Do not inflate the balloon to a pressure exceeding the rated burst pressure. (The balloon may burst and the debris may remain inside the body.)

PTCA = Percutaneous Transluminal Coronary Angioplasty, NP = Nominal Pressure, RBP = Rated Burst Pressure  
PCI = Percutaneous Coronary Intervention

For Healthcare Professionals Only.

Important information: Prior to use, refer to the instructions for use supplied with this device for indications, contraindications, suggested procedure, warnings and precautions. As part of its continuous product development policy, Cordis reserves the right to change product specifications without prior notification. Please contact your Cordis representative for additional product availability information.

RAIDEN3 Balloon is manufactured by Kaneka Corporation and distributed by Cordis. CORDIS and the Cordis LOGO are trademarks of Cordis and may be registered in the US and/or in other countries. All other marks are the property of their respective owners.  
© 2022 Cordis. All Rights Reserved. 100570120-5.

CE  
0123

