


STEP 1: ACHIEVE TEMPORARY HEMOSTASIS

INSERT DEVICE

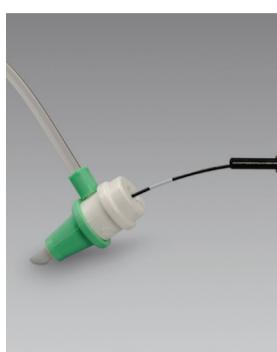

Insert the MYNXGRIP™ Vascular Closure Device into existing procedural sheath up to the white shaft marker

INFLATE THE BALLOON



Inflate the balloon until the black marker is fully visible on the inflation indicator and close stopcock


GENTLY PULL BACK TWO STOPS



- Grasp black handle and withdraw catheter until the balloon abuts the distal tip of the procedural sheath (first point of resistance)
- Continue to withdraw until the balloon abuts the arteriotomy site (second point of resistance)
- While holding adequate tension on device handle, open stopcock on procedural sheath


RESULT

TEMPORARY HEMOSTASIS IS ACHIEVED

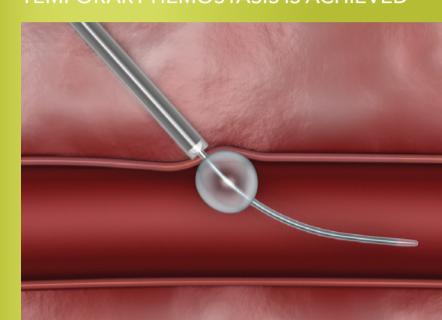


STEP 2: PLACE THE SEALANT

ADVANCE THE SEALANT

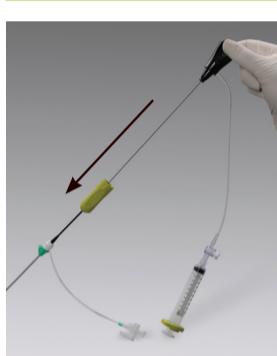


With stopcock open, detach shuttle and advance until resistance is felt

UNSHEATH THE SEALANT

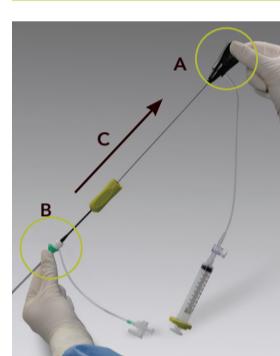

- Lighten hold on black handle
- Grasp procedural sheath and withdraw it from tissue tract
- Continue retracting until shuttle locks onto black handle


ADVANCE PAST SINGLE GREEN MARK

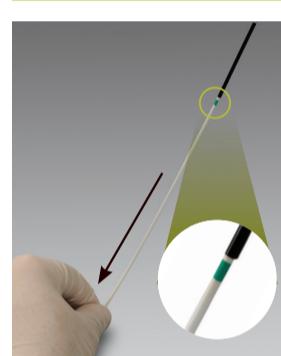

- Ensure adequate tension is employed on the black handle to keep balloon abutted against the arteriotomy and venotomy
- Immediately grasp advancer tube at skin and gently advance until single marker is fully visible
- Hold for up to 30 seconds
- Lay device down for up to 90 seconds


RESULT

SEALANT IS IN PLACE

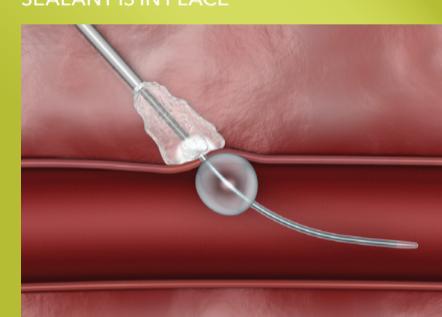

STEP 3: REMOVE THE DEVICE

LOCK, STABILIZE, DEFATE

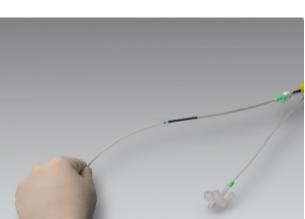

LOCK SYRINGE

- Lock syringe to maximum negative position

STABILIZE ARTERY

- Stabilize by applying light fingertip compression proximal to the insertion site
- Lightly grasp advancer tube at skin with thumb and forefinger; realign with tissue tract

DEFLATE THE BALLOON

- Open stopcock to deflate balloon
- To ensure complete balloon deflation, wait until air bubbles and fluid have stopped moving through the inflation tubing

REMOVE



REMOVE CATHETER AND ADVANCER TUBE

- Slowly withdraw catheter through the advancer tube lumen
- NOTE:** If unusual resistance is felt during catheter withdrawal, pull the advancer tube and balloon catheter together through the tissue tract
- While maintaining fingertip compression on the skin

- remove advancer tube from the tissue tract
- Fingertip compression can be applied for up to 60 seconds or as needed
- Assess for hemostasis and reapply additional fingertip compression until sterile dressing is applied and hemostasis is achieved

RESULT

PATIENT-FRIENDLY CLOSURE



PREP MYNXGRIP

REMOVE DEVICE



- Hold the MYNXGRIP™ Vascular Closure Device by the shuttle while removing from the tray
- Pull the device out of the protective tubing.

PREPARE BALLOON



- Fill locking syringe with 2-3ml of sterile saline
- Attach to stopcock and draw vacuum
- Inflate balloon until black marker on inflation indicator is fully visible
- Deflate balloon and leave syringe at neutral
- Do not remove sealant sleeve

For Healthcare Professionals Only.

Important information: Prior to use, refer to the instructions for use supplied with this device for indications, contraindications, suggested procedure, warnings and precautions. As part of its continuous product development policy, Cordis reserves the right to change product specifications without prior notification.

Please contact your Cordis representative for additional product availability information.

CORDIS, Cordis LOGO, MYNXGRIP are trademarks of Cordis and may be registered in the US and/or in other countries.

© 2024 Cordis. All Rights Reserved. 100590191-2 06/2024



2797